



PYRANOMETER

HUKSEFLUX LP02, SR11, SR12, SR20

INSTRUCTIONS

Use the following input channels on the logger to connect this sensor. See highlighted input channels marked here below. The wire colors used in the connection diagram below only applies in case the cable is supplied by Kintech Engineering.

For additional wiring & shielding information see the chapter "IMPORTANT" at the end of this dataheet.

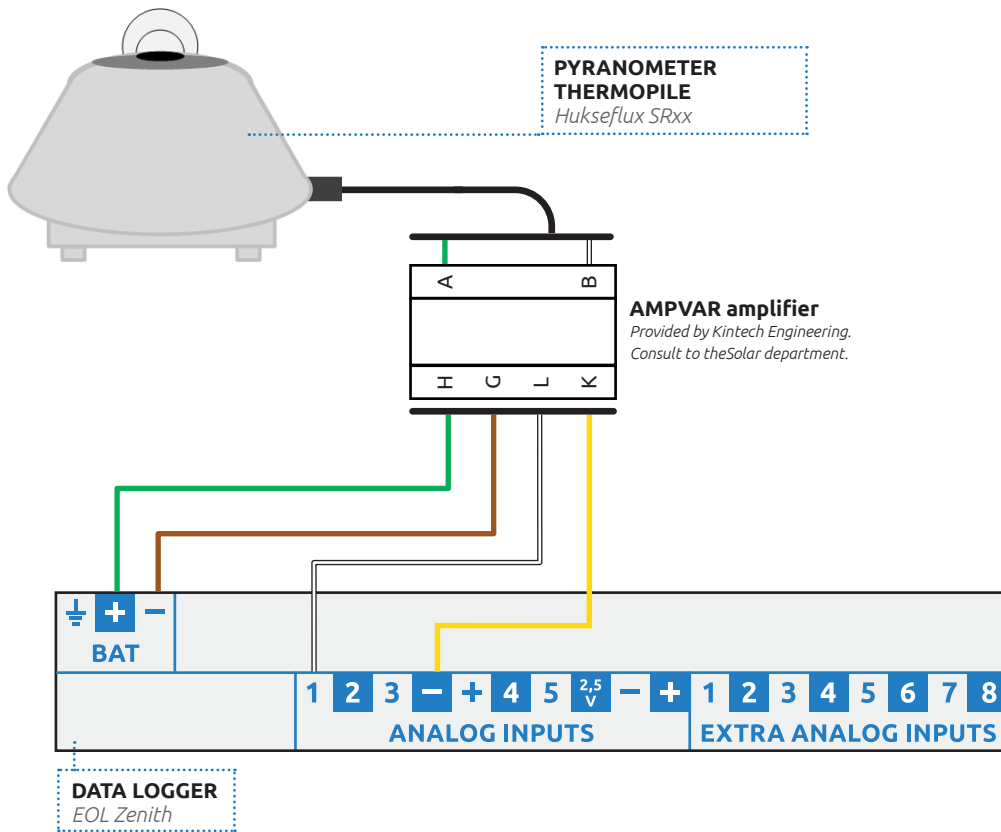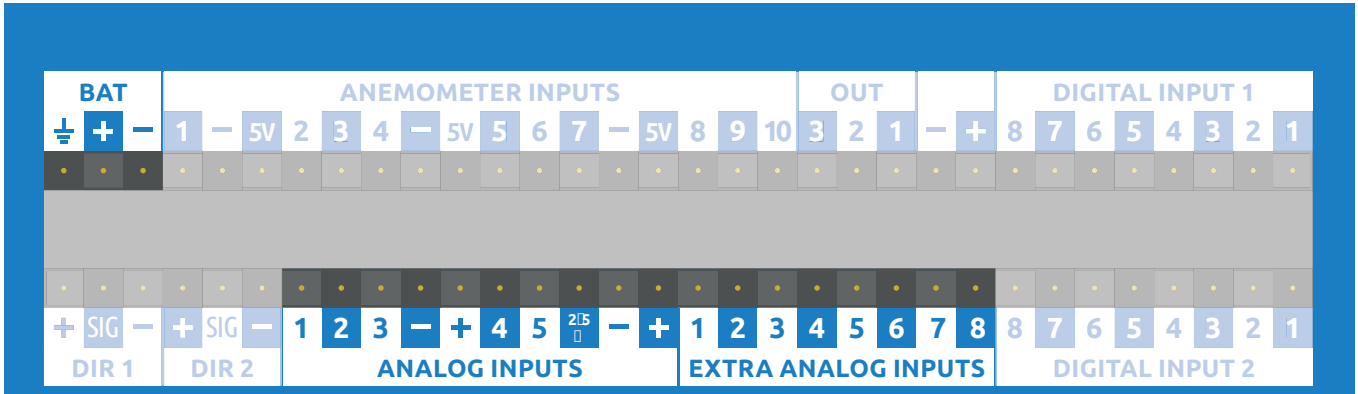

SENSOR PIN DESCRIPTION		AMPVAR AMPLIFIER		DATA LOGGER INPUT CHANNEL		KINTECH COLOR CODES	
●	Signal (-)	A					
○	Signal (+)	B					
		H	Supply (+)	BAT	(+)	●	Green
		G	Supply (-)	BAT	(-)	●	Brown
		L	Signal	ANALOG INPUTS	1	○	White
		K	Reference	ANALOG INPUTS	(-)	●	Yellow

HOW TO CONFIGURE THIS SENSOR IN EOL MANAGER

Open EOL Manager and go to the data logger you are working on. Open the “inputs” tab and select the following type and model:

- ▀ **Section:** Analog Inputs
- ▀ **Type:** Radiation
- ▀ **Model:** Thermopile

Calibration values: Tick the “Std Cal” to use this sensors standard slope and offset. If you have the Measnet calibration certificate for this sensor insert the slope and offset values from this certificate. Please note AMPVAR and Pyranometer calibration to calculate **Slope and Offset**. Consult Kintech Engineering Solar department.

Analog Inputs

Ignore	Channel	Type	Model	Units	Serial Number	Height	Boom	Username	Std Cal	Slope	Offset	Std Dev	Max
<input type="checkbox"/>	ANL1	Radiation	Thermopile	W/m2		0	0	RAD1_0_0_Ther...	<input type="checkbox"/>	0.000000	0.000000	<input type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	ANL2	---	---			0	0	Analog2	<input type="checkbox"/>	0.000000	0.000000	<input type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	ANL3	---	---			0	0	Analog3	<input type="checkbox"/>	0.000000	0.000000	<input type="checkbox"/>	<input type="checkbox"/>

SENSOR SELECTION

MODEL SELECTION

DATASHEET DOWNLOAD

CALIBRATION REQUIRED

IMPORTANT

- ▀ After configuring the sensor in EOL Manager make sure to upload the configuration file to your EOL Zenith data logger. See the “Quick User Guide” how to upload configuration files to the data logger.
- ▀ All sensor wire shields must be connected to the data logger GND terminal.
- ▀ The data logger should always be connected to a separated ground rod. **Not** to the lightning rod of the tower.
- ▀ To store data such as Std Dev, Max and Min you should tick the corresponding boxes next to each anemometer channel when setting up your site file. Otherwise these parameters will not be stored.
- ▀ It can however be distributed on all “ANALOG” and “EXTRA ANALOG” channels according to needs.

Last modified: 20.06.2017